

Independent Research Testing Center
875 Innovation Drive, Cambridge, MA 02139, USA


CERTIFICATE OF ANALYSIS (COA)

Product Name	GLP-3 RT 30 mg (Injectable Research Vial)
Chemical Name	Retatrutide (GIP/GLP-1/glucagon triple agonist)
CAS Number	2381089-83-2
Batch / Lot Number	RETA300509
Manufacturing Date	2026-08-09
Retest / Expiry Date	2028-08-09
Net Content	30 mg per vial
Storage Conditions	Store at 2–8°C, protected from light and moisture
Appearance	White to off-white lyophilized powder
Molecular Formula / MW	C221H342N46O68 / 4731.33 g/mol

Analytical Results

Test Item	Specification	Result	Method
Identification	Conforms	Conforms	LC-MS
Purity (HPLC)	≥98.0%	99.06%	HPLC
Peptide Content	95.0–105.0%	99.6%	HPLC
Appearance	White to off-white lyophilized powder	Conforms	Visual
Water Content	≤3.0%	1.1%	Karl Fischer
Heavy Metals	≤10 ppm	<10 ppm	ICP-MS
Endotoxin	<10 EU/mg	<10 EU/mg	LAL Test

HPLC Chromatogram

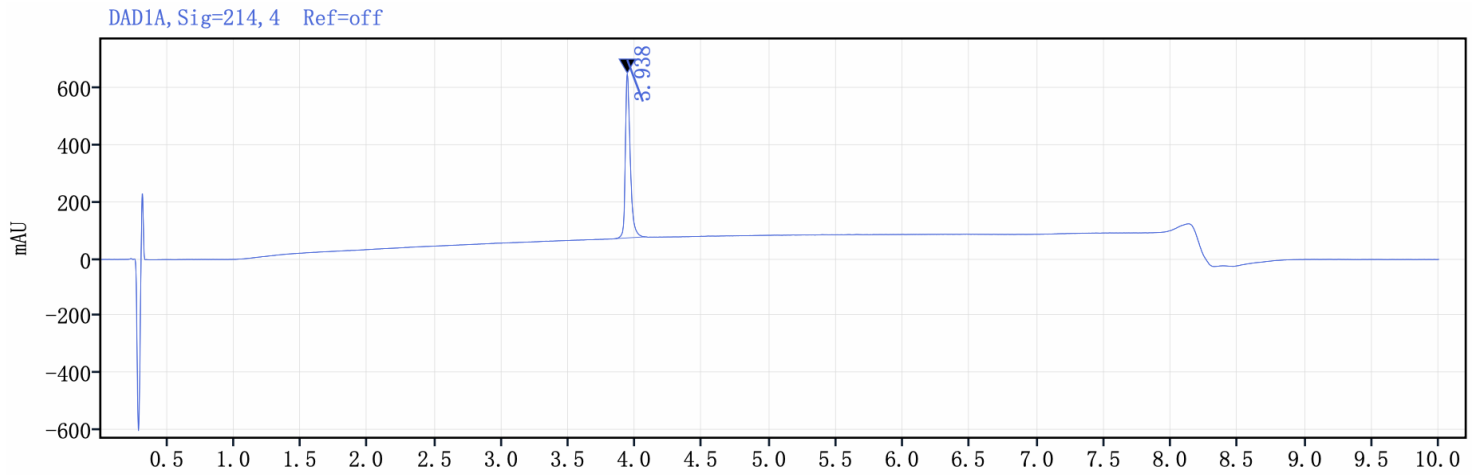

For laboratory research use only. Not for human consumption.

Tester Name	Dr. Michael Carter
Signature	<i>Michael Carter</i>
Test Date	2026-08-24